

Accepted Manuscript

Reducing radiation exposure in early-onset scoliosis surgery patients: novel use of ultrasonography to measure lengthening in magnetically-controlled growing rods

Oliver M. Stokes, MBBS, MSc, FRCS (Tr&Orth) Elizabeth J. O'Donovan, MBBS, BSc, MRCS, FRCR Dino Samartzis, DSc Cora H. Bow, MCMSc, BHS Keith D.K. Luk, MCh(Orth), MBBS, FRCSE, FRCSE, FRACS, FHKAM(Orth) Kenneth M.C. Cheung, MBBS, MD, FRCS, FHKCOS, FHKAM



PII: S1529-9430(14)00116-8

DOI: [10.1016/j.spinee.2014.01.039](https://doi.org/10.1016/j.spinee.2014.01.039)

Reference: SPINEE 55746

To appear in: *The Spine Journal*

Received Date: 8 June 2013

Revised Date: 20 December 2013

Accepted Date: 17 January 2014

Please cite this article as: Stokes OM, O'Donovan EJ, Samartzis D, Bow CH, Luk KDK, Cheung KMC, Reducing radiation exposure in early-onset scoliosis surgery patients: novel use of ultrasonography to measure lengthening in magnetically-controlled growing rods, *The Spine Journal* (2014), doi: 10.1016/j.spinee.2014.01.039.

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

**Reducing radiation exposure in early-onset scoliosis surgery patients:
novel use of ultrasonography to measure lengthening in
magnetically-controlled growing rods**

Authors: Oliver M. Stokes, MBBS, MSc, FRCS (Tr&Orth)
Elizabeth J O'Donovan, MBBS, BSc, MRCS, FRCR
Dino Samartzis, DSc
Cora H. Bow, MCMSc, BHS
Keith D.K. Luk, MCh(Orth), MBBS, FRCSE, FRCSG, FRACS, FHKAM(Orth)
Kenneth M.C. Cheung, MBBS, MD, FRCS, FHKCOS, FHKAM

Affiliations: Department of Orthopaedics and Traumatology, Duchess of Kent Children's Hospital, University of Hong Kong, Pokfulam, Hong Kong, SAR China

Disclosures: Kenneth MC Cheung has received grant and research support from Ellipse Technologies for previous studies. Oliver M Stokes has received a travel grant from Ellipse Technologies following the conclusion of this study. Ellipse Technologies purchased a 64mm ultrasound probe to facilitate image capture for this study. The authors have no other financial or competing interests to disclose in relation to this work.

Key Words: ultrasound, radiation, scoliosis, magnetic, growing-rod

Correspondence: Kenneth MC Cheung
Division of Spine Surgery
Department of Orthopaedics and Traumatology
The University of Hong Kong
Professorial Block, 5th Floor
102 Pokfulam Road
Hong Kong, SAR China
Tel: (+852) 2255-4254
Fax: (+852) 2817-4392
Email: cheungmc@hku.hk

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31

**Reducing radiation exposure in early-onset scoliosis surgery patients:
novel use of ultrasonography to measure lengthening in
magnetically-controlled growing rods**

ACCEPTED MANUSCRIPT

1 **ABSTRACT**

2

3 **Background Context:** Magnetically-controlled growing rod (MCGR) technology has been
4 reported for the treatment of early-onset scoliosis (EOS). Such technology allows for regular
5 and frequent outpatient rod distractions without the need for additional surgery. However,
6 pre- and post-distraction spine radiographs are required to verify the amount of lengthening.
7 This increased exposure to ionizing radiation in the developing child significantly increases
8 their risk profile for radiation-induced cancer and non-cancerous morbidity.

9

10 **Purpose:** This study addressed the first and novel application and reliability of the use of
11 ultrasonography, which has no ionizing radiation exposure, as an alternative to plain
12 radiographs in the visualizing and confirming of rod distractions.

13

14 **Study Design:** A prospective study.

15

16 **Patient Sample:** Six EOS patients who underwent surgical treatment with MCGRs were
17 prospectively recruited.

18

19 **Outcome Measures:** Imaging measurements based on ultrasound and plain radiographs.

20

21 **Methods:** All patients were imaged via ultrasound, ease of rod identification was established
22 and the reliability and reproducibility of optimal reference point selection assessed blindly by
23 three individuals. The clinical algorithm, using ultrasound was subsequently implemented.
24 Plain radiographs served as controls.

25

1 **Results:** Assessment of the rod's neck distance on ultrasound demonstrated a high degree of
2 inter-rater reliability ($\alpha=0.99$; $p<0.001$). Intra-rater reliability remained high on repeat
3 measurements at different time intervals ($\alpha=1.00$; $p<0.001$). Satisfactory inter-rater reliability
4 was noted when measuring the rod's neck ($\alpha=0.73$; $p=0.010$) and high reliability was noted in
5 assessing the housing of the rod ($\alpha=0.85$; $p=0.01$) on plain radiographs. Under blinded
6 conditions 2mm rod distraction measured on radiographs corresponded to 1.7mm distraction
7 on ultrasound (SD: 0.24mm; $p<0.001$). Subsequently the clinical algorithm using ultrasound,
8 instead of radiographs, has been successfully implemented.

9
10 **Conclusions:** This is the first study to report the use of a novel technique using non-invasive,
11 non-ionizing ultrasound to reliably document rod distractions in EOS patients. A high-level
12 of inter- and intra-rater reliability was noted. More importantly, the use of ultrasonography
13 may result in fewer whole spine radiographs from being taken in patients who have had
14 MCGRs implanted for EOS; thereby decreasing their exposure to ionizing radiation and the
15 potential risk of future radiation-induced diseases.

16
17 **Level of Evidence:** Level II diagnostic study.

18
19
20
21
22
23
24
25

1 INTRODUCTION

2

3 Scoliosis is a three-dimensional deformity^{1,2} of the spine, characterized by lateral
4 deviation in the coronal plane. The majority of patients require no treatment, however, in a
5 small subset, the lack of appropriate treatment can lead to compromise of pulmonary function
6 and unacceptable cosmesis.³⁻⁵ Early-onset scoliosis (EOS) begins before the age of 5 years
7 and is independent of aetiology,⁶ which includes both congenital and idiopathic infantile
8 types. Spinal deformity at this young an age presents a particular challenge as the spine,
9 thoracic cage and its contents are all growing rapidly. As such, the thorax cannot support
10 normal lung maturation and respiration.⁷ In order to prevent progression of spinal deformity,
11 bracing, casting and spinal fusion have all been employed,⁸⁻¹⁰ but conservative measures fail
12 to prevent progression in young patients.⁸⁻¹⁰ In addition, spinal fusion in the skeletally
13 immature child will result in loss of normal spinal growth⁸⁻¹⁰ with consequent poor
14 respiratory and cosmetic effects.¹¹

15 Growing rods are spinal implants that guide spinal growth. They have been used in
16 order to address the limitations of both bracing and surgery in patients with EOS.¹²⁻¹⁶
17 Traditionally, distraction (i.e. lengthening of the rods) of these systems required invasive,
18 open surgery under general anesthesia every 6 months until skeletal maturity is reached. Such
19 a frequent procedure can lead to potential intraoperative complications, repeat
20 hospitalization, increased health-care costs, and psychological impact for the child and
21 parent.^{5,17} In order to minimize the limitations of this procedure to patients and their
22 families, a magnetically-controlled growing rod (MCGR) system was developed, which had
23 been validated in animals¹⁸ and its safety and efficacy has been noted in humans.^{18,19}

24 With the use of the MCGR system, distraction can take place regularly and potentially
25 frequently in the outpatient clinic, in order to more closely mimic normal growth of the spine.

1 At the authors' institution, we have distracted the implant on a monthly basis, with
2 distractions of approximately 2mm at each visit to parallel normal physiologic growth.
3 However, such frequent distractions may inconvenience the parent and child. More
4 importantly, distraction is measured and documented through the use of pre-distraction and
5 post-distraction plain radiographs, which has led to concerns about the amount of ionizing
6 radiation exposure in children. Ionizing radiation is known to cause cell death and genetic
7 mutation, and is associated with cancerous and noncancerous disease.^{20, 21} In fact, excess
8 amounts of ionizing radiation exposure in children with scoliosis has led to the development
9 of breast cancer and increased mortality.²²⁻²⁴

10 Ultrasound is a non-invasive, non-ionizing imaging modality with increasing scope of
11 applications, including the measurement of stents implanted in the human body,²⁵ the
12 relationship of nerves to orthopedic implants²⁶ and the evaluation of mobile bearings in knee
13 arthroplasty.²⁷ The use of ultrasound scanning had been reported in the measurement of leg-
14 length discrepancy,²⁸ assessment of new bone formation during limb lengthening,²⁹ and
15 measurement of fetal spine length in utero.³⁰

16 As such, in an attempt to reduce the number of plain radiographs required to monitor
17 and chart the distraction of the MCGRs, the following study was undertaken to determine the
18 feasibility and reproducibility of the novel use of ultrasonography to measure rod
19 distractions.

20

21

22 **MATERIALS AND METHODS**

23

24 Six patients who have been treated with the MCGR for scoliosis were volunteered by
25 their parents to participate in the study, and informed consent was taken, when they attended

1 for routine outpatient lengthening at a single institution. They had a mean age of 12.5 years
2 (range: 8 – 16 years). There were 2 males and 4 females. The diagnoses of these cases were
3 idiopathic scoliosis (n=2), neurofibromatosis (n=1), Ehlers-Danlos Syndrome (n=1),
4 Noonan's syndrome (n=1) and Charge syndrome (n=1).

5 In order to standardize the ultrasound technique, the patients were all positioned on
6 the couch in the same manner (**Figure 1**). The ultrasound images were obtained using either
7 one of 2 machines: the Logiq500 V/R 4.10, GE Medical Systems (Buckinghamshire, U.K.)
8 and the SonoSite TITAN 38 Linear Array probe, Universal Diagnostic Solutions (California,
9 U.S.A.). Between each ultrasound image that was acquired, the investigator removed the
10 ultrasound probe from the patient by a distance of greater than 10cm.

11 Using the ultrasound probe the investigator located the implant housing and then the
12 extended portion of the rod (**Figure 2**). The ultrasound probe was then gently manipulated
13 until an optimal image was obtained. This image was then measured on the ultrasound
14 machine. An optimal image includes visualization of the housing, the acoustic shadow that it
15 casts, the hyperechoic rod and the terminal reference point and the acoustic shadow cast by it
16 (**Figure 3**).

17

18 *Study 1. Optimum Reference Point Selection.*

19 When radiographs were used to measure distraction of the MCGRs, the measurements
20 were made directly from the distraction mechanism (**Figure 4**). The distraction mechanism is
21 however housed in titanium and therefore not visible on ultrasound. Consequently, the
22 MCGR had to be measured from the end of the titanium housing to another reference point
23 on the rod. Nine ultrasound images were obtained and measured by a single investigator with
24 the screw as a reference point and 9 further images were obtained and measured with the
25 neck of the rod as a reference point (**Figure 5**).

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25

Study 2. Intra-Rater Reliability

To test the reliability of ultrasound to measure the extended portion of the rod, a single investigator measured the rod on a single patient 5 times. The patient then stood up, before returning to the examination couch and 5 further measurements were obtained. Finally, a set of 5 measurements, were obtained with the patient standing up between each measurement. A total of 15 measurements were made to test the intra-rater reliability of the protocol.

Study 3. Inter-Rater Repeatability

Following the development of the protocol (study 1) and training of 2 other investigators, the reproducibility of ultrasound to measure the extended portion of the rod was tested. Three investigators measured the rod 5 times each, on 3 patients.

Study 4. Demonstration of Lengthening

The use of ultrasound to measure lengthening of MCGRs was demonstrated by a single investigator on 4 patients on 1 occasion and then more than 30 days later a second investigator repeated the demonstration on 3 patients. Both investigators were blinded to whether the rods were distracted and by how much. On both occasions, in all of the cases, the measurements obtained using ultrasound were compared to measurements made from pre and post distraction plain radiographs. The measurements from the radiographs served as controls for this study.

1 ***Study 5. Repeatability of Delayed Reference Point Selection***

2 Compounding the potential error in obtaining images of MCGRs using ultrasound, an
3 additional potential error in determination of length is the measurement of the images
4 obtained. In order to address this, a single investigator re-measured 3 of the images from
5 Study 4 using ImageJ 1.46r (National Institutes of Health, USA. <http://imagej.nih.gov/ij>).
6 Each image was measured 10 times on 3 occasions, separated by 72 hours.

8 ***Study 6. Measurement of MCGR on Plain Radiographs***

9 In order to compare the reliability of ultrasound to plain radiograph for measurement
10 of the rods, 2 investigators measured a single radiograph, on maximal magnification, using
11 Centricity PACS (GE Healthcare). Each investigator measured the image in the conventional
12 manner 5 times by measuring the expanded portion in the housing, and then measured 5
13 times between the 2 reference points being used in the ultrasound protocol (**Figure 4**). These
14 measurements were repeated on 3 occasions, separated by more than 72 hours. This part of
15 the study was undertaken to validate the use of radiographs as controls for the use of
16 ultrasound for the measurement of lengthening of MCGRs and to validate the housing as the
17 most reliable portion of the MCGR to be measured when using plain radiographs.

19 ***Statistical Analysis***

20 All statistical analysis was performed by a single investigator. Mean and standard
21 deviations were obtained where appropriate. Alpha values were assessed to determine the
22 strength of reliability. Intra- and inter-rater reliabilities were performed by assessing
23 Cronbach's alpha with the analyses of intraclass correlations to obtain 95% confidence
24 intervals (CI). The threshold of significance was established at $p < 0.05$. Cronbach's alpha
25 values less than 0.69 were regarded as poor, values of 0.70 to 0.79 were considered

1 satisfactory, and values equal or greater than 0.80 were considered as exhibiting good to high
2 reliability.³¹

3

4 **RESULTS**

5

6 One patient was selected to determine the optimum reference point on ultrasound.

7 Over nine sets of measurement, the mean screw distance was 14.04mm (SD: 0.27mm) and
8 the mean neck of the rod distance was 8.31mm (SD: 0.12mm) on the MCGR (**Figure 5**).

9 Since the variance was less in the distance of the rod's neck, this reference point was selected
10 as the most optimal.

11 With respect to inter-rater reliability, assessment of the rod's neck distance on
12 ultrasound was performed in 3 patients, demonstrating a high degree of reliability ($\alpha=0.99$;
13 95% CI: 0.99-1.00; $p<0.001$). Intra-rater reliability remained high on repeat measurements at
14 different time intervals ($\alpha=1.00$; 95% CI: 1.00 - 1.00; $p<0.001$). Satisfactory inter-rater
15 reliability was noted when measuring the rod's neck on plain radiographs ($\alpha=0.73$; 95% CI:
16 0.19-0.91; $p=0.010$) and high reliability was noted in assessing the housing of the rod
17 ($\alpha=0.85$; 95% CI: 0.49-0.95; $p=0.01$). In the assessment of distraction on ultrasound
18 compared to actual distraction based on plain radiographs (controls), we noted that when the
19 rod showed distraction on x-rays of 2mm, the mean distraction measured on ultrasound was a
20 mean of 1.7mm (SD: 0.24mm; $p<0.001$). In contrast, in scenarios where no distraction of the
21 rod was noted on plain radiographs, the ultrasound measurements showed no significant
22 difference (mean = 0.52mm, SD: 0.33mm; $p=0.20$). As such, the findings suggest that
23 distraction of the rods as noted on plain radiographs can be observed on ultrasound (**Figure**
24 **6A-D**).

25

1 DISCUSSION

2

3 This study is, to our knowledge, the first to explore the use of ultrasonography to
4 measure changes in spinal implant length. In order to demonstrate its feasibility and
5 reliability, we first identified reproducible reference points on the implant that could be used
6 for measurements. We then demonstrated that these measurements had good intra- and inter-
7 observer reliability, and that they were comparable to measurements taken from radiographs.

8 The reliability of ultrasonography to measure an implant *in vivo* is dependent on
9 minimizing 2 potential sources of error: (1) the acquisition of the image and (2) the selection
10 of the reference points (measurement of the acquired image). Optimal image acquisition
11 requires training, attention to detail and rejection of sub-optimal image quality (i.e. images
12 without clarity of reference points and with any loss of image capture between the reference
13 points). The higher intra-rater agreeability demonstrated by the radiologist compared to the
14 other raters is probably a reflection of her familiarity and training in this imaging modality
15 and her ability to capture an ideal image more easily. The results from Study 1 showed that
16 the optimal terminal reference point was the transition point, or neck in the extended portion
17 of the rod and not the pedicle screw used to fix the MCGR to the spine. We postulate that this
18 is due to the larger and possibly more inconsistent acoustic shadow cast by the larger pedicle
19 screw, compared to the transition portion of the rod. During this study, and subsequently
20 when this technique has been used to document lengthening of MCGRs in the clinic, accurate
21 determination of the terminal reference point (transition point / neck of extended portion of
22 the rod) was difficult in the hands of less experienced investigators when the pedicle screw
23 was sited less than 1cm from the terminal reference point. Therefore, in our institution we
24 now recommend that all pedicle screws are placed more than 1.5cm from the transition point
25 in the extended portion of the rod.

1 The traditional method of measuring and documenting lengthening of MCGRs is
2 using plain radiographs.¹⁹ Two raters measured the extended portion of the rod (as used in
3 the ultrasonography technique reported in this study) and the housing of the implant (how
4 extension of MCGRs has been measured on plain radiographs previously) on a single
5 radiography, 5 times, repeated on 3 occasions, separated by more than 72 hours. This was
6 done because radiographs are gold standard images used to document lengthening of growing
7 rods, as such, they were used as the controls in this study. Additionally this allowed the
8 housing, as opposed to the neck of the rod, to be validated as the optimal region in which to
9 measure lengthening of MCGRs on plain radiographs. The results show that measuring the
10 MCGR housing is more repeatable and reliable. This is due to the ease of reference point
11 selection in the housing. Throughout the study and subsequently when the methodology was
12 demonstrated, radiographs more accurately documented lengthening, but measurements with
13 ultrasound had a narrower distribution of measurements. The higher accuracy of MCGR
14 measurements with plain radiograph compared to ultrasonography was also likely to be in
15 part due to radiographs being measured under 200% magnification and ultrasound being
16 measured without magnification. In our institution, the ultrasound machines were not linked
17 to a viewer with DICOM imaging capabilities and, as such, all measurements were performed
18 in real-time on the ultrasound machines. In institutions with more integrated imaging
19 facilities that are able to measure ultrasonography under magnification, greater accuracy is
20 anticipated. To test whether reference point selection was repeatable, a single investigator
21 measured 3 ultrasounds using ImageJ on 3 separate occasions, separated by more than 72
22 hours. A high-level of intra-rater agreeability was demonstrated.

23 The primary purpose of this study was to develop a methodology to reduce the
24 amount of radiation exposure in immature patients undergoing serial out-patient lengthening
25 of MCGRs. Radiation exposure in children is associated with radiation-induced cancer^{24, 32-36}

1 and as few as 25 whole spine radiographs have been reported to increase the risk of breast
2 cancer by 70%.²⁴ MCGRs could be lengthened on a monthly basis, and have been implanted
3 in patients as young as 5 years and 8 months old.¹⁹ Monthly lengthening, accompanied by
4 documentation of lengthening using plain radiographs until skeletal maturity would
5 necessitate considerably more than 25 whole spine radiographs and may therefore result in
6 further excess risk of cancer compared to the general population. If a MCGRs was implanted
7 in a patient of 5-years old, who was subsequently lengthened on a monthly basis for 8-years,
8 with pre and post distraction radiographs then they would receive 192 whole spine
9 radiographs. This study offers an alternative method to measure and document lengthening of
10 MCGRs.

11 Furthermore, the findings of this study have been reported back to the implant
12 manufacturer (Ellipse Technologies). We have suggested a potential future modification of
13 the implant that may entail a metal ring being affixed or bonded at the transition point on the
14 neck of the rod, which would not affect the torsional or bending rigidity of the implant. Such
15 a modification would allow easier terminal reference point identification using this
16 ultrasound technique and would likely improve the accuracy and ease of measurement of
17 MCGRs.

18 This study has shown that the technique is easily learned and is acceptable to patients.
19 It took an average of 35 seconds to locate the rod using ultrasound, 9 seconds to capture each
20 image and 10 seconds to measure the rod. At our institution, the ultrasound machine is
21 located in a room adjacent to the room where the patients undergo MCGR lengthening. This
22 setup and novel technique is a further advantage to our patients for their convenience of not
23 having to go to the radiology department and potentially have further waiting time before
24 having plain radiographs taken. Ultrasound scanning is available in most hospitals and is
25 relatively cheap. In our institution, the ultrasound imaging for these patients is being

1 performed by a basic scientist, under the supervision of an orthopedic spinal surgeon;
2 therefore, not placing any additional burden on the radiology department. Furthermore, this
3 technique has the potential for translation to other applications. For example, the
4 measurement of traditional growing rod constructs in spinal surgery and for the measurement
5 of magnetically-controlled endoprotheses for treatment of malignant bone tumors in
6 skeletally immature children.

7

8 *Limitations for the Use of Ultrasound*

9 Compared to the current standard of radiography, ultrasound scanning, however, does not
10 allow for the assessment of fusion blocks at the proximal and distal fixation points of the
11 MCGRs, nor does it allow the implants themselves to be assessed for other potential
12 complications, such as loosening or implant failure. In addition, correlation of plain
13 radiographs to spinal balance is helpful in the assessment and differential lengthening in
14 some of these patients. Therefore, in our institution, while we no longer use plain radiographs
15 to measure and document lengthening of MCGRs and have adopted the use of
16 ultrasonography to measure rod lengthening, we intend to continue to take a plain radiograph
17 every 6 months post-implantation, with the hope of possibly reducing the frequency of
18 ionizing radiation exposure associated with plain radiographs.

19 A potential limitation of this technique is the size of the ultrasound probe used to
20 capture the images. We used a 64mm probe in this study. Probes of this size are
21 commercially available. The current design of the MCGRs can only be lengthened to a
22 maximum of 48mm, hence the decision to purchase a probe of this width. Certainly at the
23 initial period after surgery, when the implant has not been distracted so much, smaller US
24 probes can be used. Alternatively if future designs of MCGR allows lengthening beyond

1 64mm, larger ultrasound probes, or an alternative methodology, such as the use of panoramic
2 ultrasound,³⁷ will need to be used.

3

4 **CONCLUSIONS**

5

6 Our study is the first, to our knowledge, to demonstrate the reliability of using
7 ultrasound technology to assess rod lengthening in patients with EOS undergoing surgical
8 treatment with the MCGR. This practical and easy to administer technique can change
9 clinical practice by decreasing the frequency of plain radiographs and the associated
10 cumulative ionizing radiation exposure in the developing child.

11

12

13

14

15

16

17

18

19

20

21

22

23

24

25

1 SOURCE OF FUNDING

2

3 Ellipse Technologies Incorporated purchased a 64mm ultrasound probe to facilitate
4 image capture for this study. Ellipse Technologies Incorporated was not involved in any of
5 the surgical procedures, distractions, ultrasound assessments, data collection, analysis or
6 interpretation of the results, writing or editing of the manuscript, or the decision to submit the
7 study for publication.

8

9

10

11

12

13

14

15

16

17

18

19

20

21

22

23

24

25

1 **RERERENCES**

2

3 **1.** Kojima T, Kurokawa T. Quantitation of three-dimensional deformity of idiopathic
4 scoliosis. *Spine* 1992; 17: S22-9.

5 **2.** Stokes IA, Bigalow LC, Moreland MS. Three-dimensional spinal curvature in
6 idiopathic scoliosis. *Journal of orthopaedic research : official publication of the*
7 *Orthopaedic Research Society* 1987; 5: 102-13.

8 **3.** James JJ. Idiopathic scoliosis; the prognosis, diagnosis, and operative indications
9 related to curve patterns and the age at onset. *The Journal of bone and joint surgery*
10 *British volume* 1954; 36-B: 36-49.

11 **4.** James JJ, Lloyd-Roberts GC, Pilcher MF. Infantile structural scoliosis. *The Journal of*
12 *bone and joint surgery British volume* 1959; 41-B: 719-35.

13 **5.** Bess S, Akbarnia BA, Thompson GH, et al. Complications of growing-rod treatment
14 for early-onset scoliosis: analysis of one hundred and forty patients. *The Journal of*
15 *bone and joint surgery American volume* 2010; 92: 2533-43.

16 **6.** Gillingham BL, Fan RA, Akbarnia BA. Early onset idiopathic scoliosis. *The Journal*
17 *of the American Academy of Orthopaedic Surgeons* 2006; 14: 101-12.

18 **7.** Campbell RM, Jr., Smith MD, Mayes TC, et al. The characteristics of thoracic
19 insufficiency syndrome associated with fused ribs and congenital scoliosis. *The*
20 *Journal of bone and joint surgery American volume* 2003; 85-A: 399-408.

21 **8.** McMaster MJ, Macnicol MF. The management of progressive infantile idiopathic
22 scoliosis. *The Journal of bone and joint surgery British volume* 1979; 61: 36-42.

23 **9.** Mehta MH. Growth as a corrective force in the early treatment of progressive
24 infantile scoliosis. *The Journal of bone and joint surgery British volume* 2005; 87:
25 1237-47.

- 1 **10.** Robinson CM, McMaster MJ. Juvenile idiopathic scoliosis. Curve patterns and
2 prognosis in one hundred and nine patients. *The Journal of bone and joint surgery*
3 *American volume* 1996; 78: 1140-8.
- 4 **11.** Goldberg CJ, Gillic I, Connaughton O, et al. Respiratory function and cosmesis at
5 maturity in infantile-onset scoliosis. *Spine* 2003; 28: 2397-406.
- 6 **12.** Akbarnia BA, Breakwell LM, Marks DS, et al. Dual growing rod technique followed
7 for three to eleven years until final fusion: the effect of frequency of lengthening.
8 *Spine* 2008; 33: 984-90.
- 9 **13.** Akbarnia BA, Marks DS, Boachie-Adjei O, Thompson AG, Asher MA. Dual growing
10 rod technique for the treatment of progressive early-onset scoliosis: a multicenter
11 study. *Spine* 2005; 30: S46-57.
- 12 **14.** Winter RB, Moe JH, Lonstein JE. Posterior spinal arthrodesis for congenital scoliosis.
13 An analysis of the cases of two hundred and ninety patients, five to nineteen years
14 old. *The Journal of bone and joint surgery American volume* 1984; 66: 1188-97.
- 15 **15.** Elsebai HB, Yazici M, Thompson GH, et al. Safety and efficacy of growing rod
16 technique for pediatric congenital spinal deformities. *Journal of pediatric orthopedics*
17 2011; 31: 1-5.
- 18 **16.** Thompson GH, Akbarnia BA, Campbell RM, Jr. Growing rod techniques in early-
19 onset scoliosis. *Journal of pediatric orthopedics* 2007; 27: 354-61.
- 20 **17.** Caldas JC, Pais-Ribeiro JL, Carneiro SR. General anesthesia, surgery and
21 hospitalization in children and their effects upon cognitive, academic, emotional and
22 sociobehavioral development - a review. *Paediatric anaesthesia* 2004; 14: 910-5.
- 23 **18.** Akbarnia BA, Cheung K, Noordeen H, et al. Next Generation of Growth-Sparing
24 Technique: Preliminary Clinical Results of a Magnetically Controlled Growing Rod
25 (MCGR) in 14 Patients With Early Onset Scoliosis. *Spine* 2012.

- 1 **19.** Cheung KM, Cheung JP, Samartzis D, et al. Magnetically controlled growing rods for
2 severe spinal curvature in young children: a prospective case series. *Lancet* 2012;
3 379: 1967-74.
- 4 **20.** Preston DL, Ron E, Tokuoka S, et al. Solid cancer incidence in atomic bomb
5 survivors: 1958-1998. *Radiation research* 2007; 168: 1-64.
- 6 **21.** Baker JE, Moulder JE, Hopewell JW. Radiation as a risk factor for cardiovascular
7 disease. *Antioxidants & redox signaling* 2011; 15: 1945-56.
- 8 **22.** Ronckers CM, Land CE, Miller JS, Stovall M, Lonstein JE, Doody MM. Cancer
9 mortality among women frequently exposed to radiographic examinations for spinal
10 disorders. *Radiation research* 2010; 174: 83-90.
- 11 **23.** Ronckers CM, Doody MM, Lonstein JE, Stovall M, Land CE. Multiple diagnostic X-
12 rays for spine deformities and risk of breast cancer. *Cancer epidemiology, biomarkers*
13 *& prevention : a publication of the American Association for Cancer Research,*
14 *cosponsored by the American Society of Preventive Oncology* 2008; 17: 605-13.
- 15 **24.** Doody MM, Lonstein JE, Stovall M, Hacker DG, Luckyanov N, Land CE. Breast
16 cancer mortality after diagnostic radiography: findings from the U.S. Scoliosis Cohort
17 Study. *Spine* 2000; 25: 2052-63.
- 18 **25.** He Y, Maehara A, Mintz GS, et al. Intravascular ultrasound assessment of cobalt
19 chromium versus stainless steel drug-eluting stent expansion. *The American journal*
20 *of cardiology* 2010; 105: 1272-5.
- 21 **26.** Livani B, Belangero W, Andrade K, Zuiani G, Pratali R. Is MIPO in humeral shaft
22 fractures really safe? Postoperative ultrasonographic evaluation. *International*
23 *orthopaedics* 2009; 33: 1719-23.

- 1 **27.** Aigner C, Radl R, Pechmann M, Rehak P, Stacher R, Windhager R. The accuracy of
2 ultrasound for measurement of mobile- bearing motion. *Clinical orthopaedics and*
3 *related research* 2004; 169-74.
- 4 **28.** Krettek C, Koch T, Henzler D, Blauth M, Hoffmann R. [A new procedure for
5 determining leg length and leg length inequality using ultrasound. II: Comparison of
6 ultrasound, teleradiography and 2 clinical procedures in 50 patients]. *Der*
7 *Unfallchirurg* 1996; 99: 43-51.
- 8 **29.** Eyres KS, Bell MJ, Kanis JA. Methods of assessing new bone formation during limb
9 lengthening. Ultrasonography, dual energy X-ray absorptiometry and radiography
10 compared. *The Journal of bone and joint surgery British volume* 1993; 75: 358-64.
- 11 **30.** Ulm MR, Kratochwil A, Oberhuemer U, Ulm B, Blaicher W, Bernaschek G.
12 Ultrasound evaluation of fetal spine length between 14 and 24 weeks of gestation.
13 *Prenatal diagnosis* 1999; 19: 637-41.
- 14 **31.** Vangeneugden T, Laenen A, Geys H, Renard D, Molenberghs G. Applying concepts
15 of generalizability theory on clinical trial data to investigate sources of variation and
16 their impact on reliability. *Biometrics* 2005; 61: 295-304.
- 17 **32.** Samartzis D, Nishi N, Hayashi M, et al. Exposure to ionizing radiation and
18 development of bone sarcoma: new insights based on atomic-bomb survivors of
19 Hiroshima and Nagasaki. *The Journal of bone and joint surgery American volume*
20 2011; 93: 1008-15.
- 21 **33.** Hawkins MM. Second primary tumors following radiotherapy for childhood cancer.
22 *International journal of radiation oncology, biology, physics* 1990; 19: 1297-301.
- 23 **34.** Tucker MA, D'Angio GJ, Boice JD, Jr., et al. Bone sarcomas linked to radiotherapy
24 and chemotherapy in children. *The New England journal of medicine* 1987; 317: 588-
25 93.

- 1 **35.** Le Vu B, de Vathaire F, Shamsaldin A, et al. Radiation dose, chemotherapy and risk
2 of osteosarcoma after solid tumours during childhood. *International journal of cancer*
3 *Journal international du cancer* 1998; 77: 370-7.
- 4 **36.** Bechler JR, Robertson WW, Jr., Meadows AT, Womer RB. Osteosarcoma as a
5 second malignant neoplasm in children. *The Journal of bone and joint surgery*
6 *American volume* 1992; 74: 1079-83.
- 7 **37.** Weng L, Tirumalai AP, Lowery CM, et al. US extended-field-of-view imaging
8 technology. *Radiology* 1997; 203: 877-80.

9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25

1 **FIGURE LEGENDS**

2

3 **Figure 1:** Photograph of a patient lying prone on the examination table with his arms
4 stretched out in front of him and a pillow under positioned under the upper thorax for
5 comfort.

6

7 **Figure 2:** Photograph of the MCGR. The blue arrow points to the motor (which drives the
8 rod lengthening). The housing is between the 2 yellow arrows, this is the portion of the rod
9 that is first identified by ultrasound. The extended portion of the rod lies to the left of the
10 housing. The neck, or transition point of the rod, is identified by the white arrow. The change
11 in the dimensions of the rod in this region results in a change in the intensity of the
12 hyperechoic ultrasound representation of the rod and an associated acoustic shadow.

13

14 **Figure 3:** Ultrasound image of the MCGR. The yellow arrow points to the terminal portion
15 of the housing and the acoustic shadow that it casts. The white arrow points to the neck of the
16 rod and the acoustic shadow that it casts. The red arrow points to the pedicle screw, used to
17 fix the MCGR to the spine, and the acoustic shadow that it casts.

18

19 **Figure 4:** Plain radiograph showing how distraction of the MCGR has been measured prior
20 to this study (green line and corresponding measurement). The amount of distraction was
21 measured directly from the expansion of the extension mechanism. The yellow line and
22 corresponding measurement indicated the portion of the rod that was measured by ultrasound.

23

24 **Figure 5:** The MCGR implanted in a spinal model. The yellow arrow points to the terminal
25 portion of the housing. The white arrow points to the neck of the rod, this is the point where

1 the rod diameter changes. The red arrow points to the pedicle screw, used to fix the MCGR to
2 the spine.

3


4 **Figure 6:** (A) Plain radiograph showing 2 MCGRs implanted into a patient. The radiograph
5 was taken prior to distraction. The housing of the left MCGR measured 27.9mm prior to
6 distraction. (B) Ultrasound image of the extended portion (measuring 35.1mm between the 2
7 reference points) of the left MCGR, in the same patient, prior to distraction. (C) Plain
8 radiograph showing 2 MCGRs implanted in the same patient following distraction. The
9 housing measured 29.6mm post distraction. Extension of the left MCGRs as measured from
10 distraction from within the housing (grey line) was 1.7mm. (D) Ultrasound image of the
11 extended portion (measuring 36.8mm between the 2 reference points) of the left MCGR, in
12 the same patient, following the distraction. The extended portion of the rod was measured to
13 have lengthened by 1.7mm using this imaging modality.




ACCEPTED MANUSCRIPT




ACCEPTED MANUSCRIPT

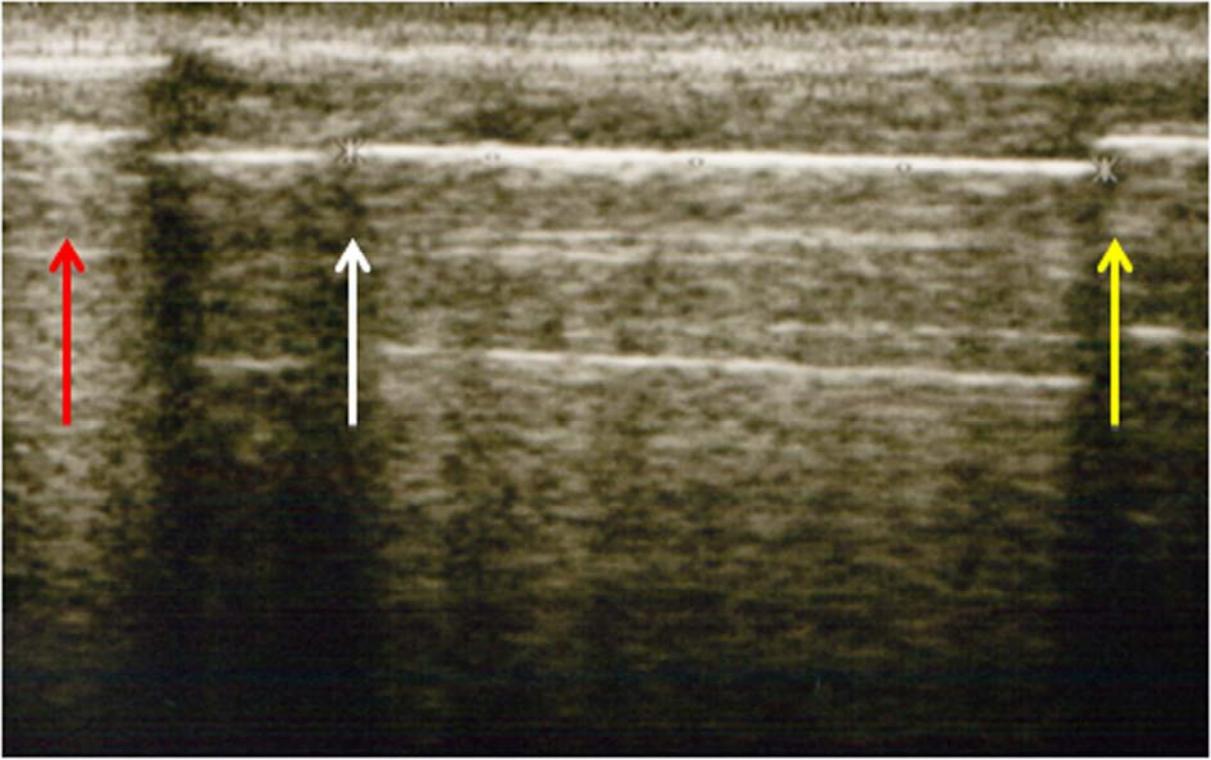


ACCEPTED MANUSCRIPT

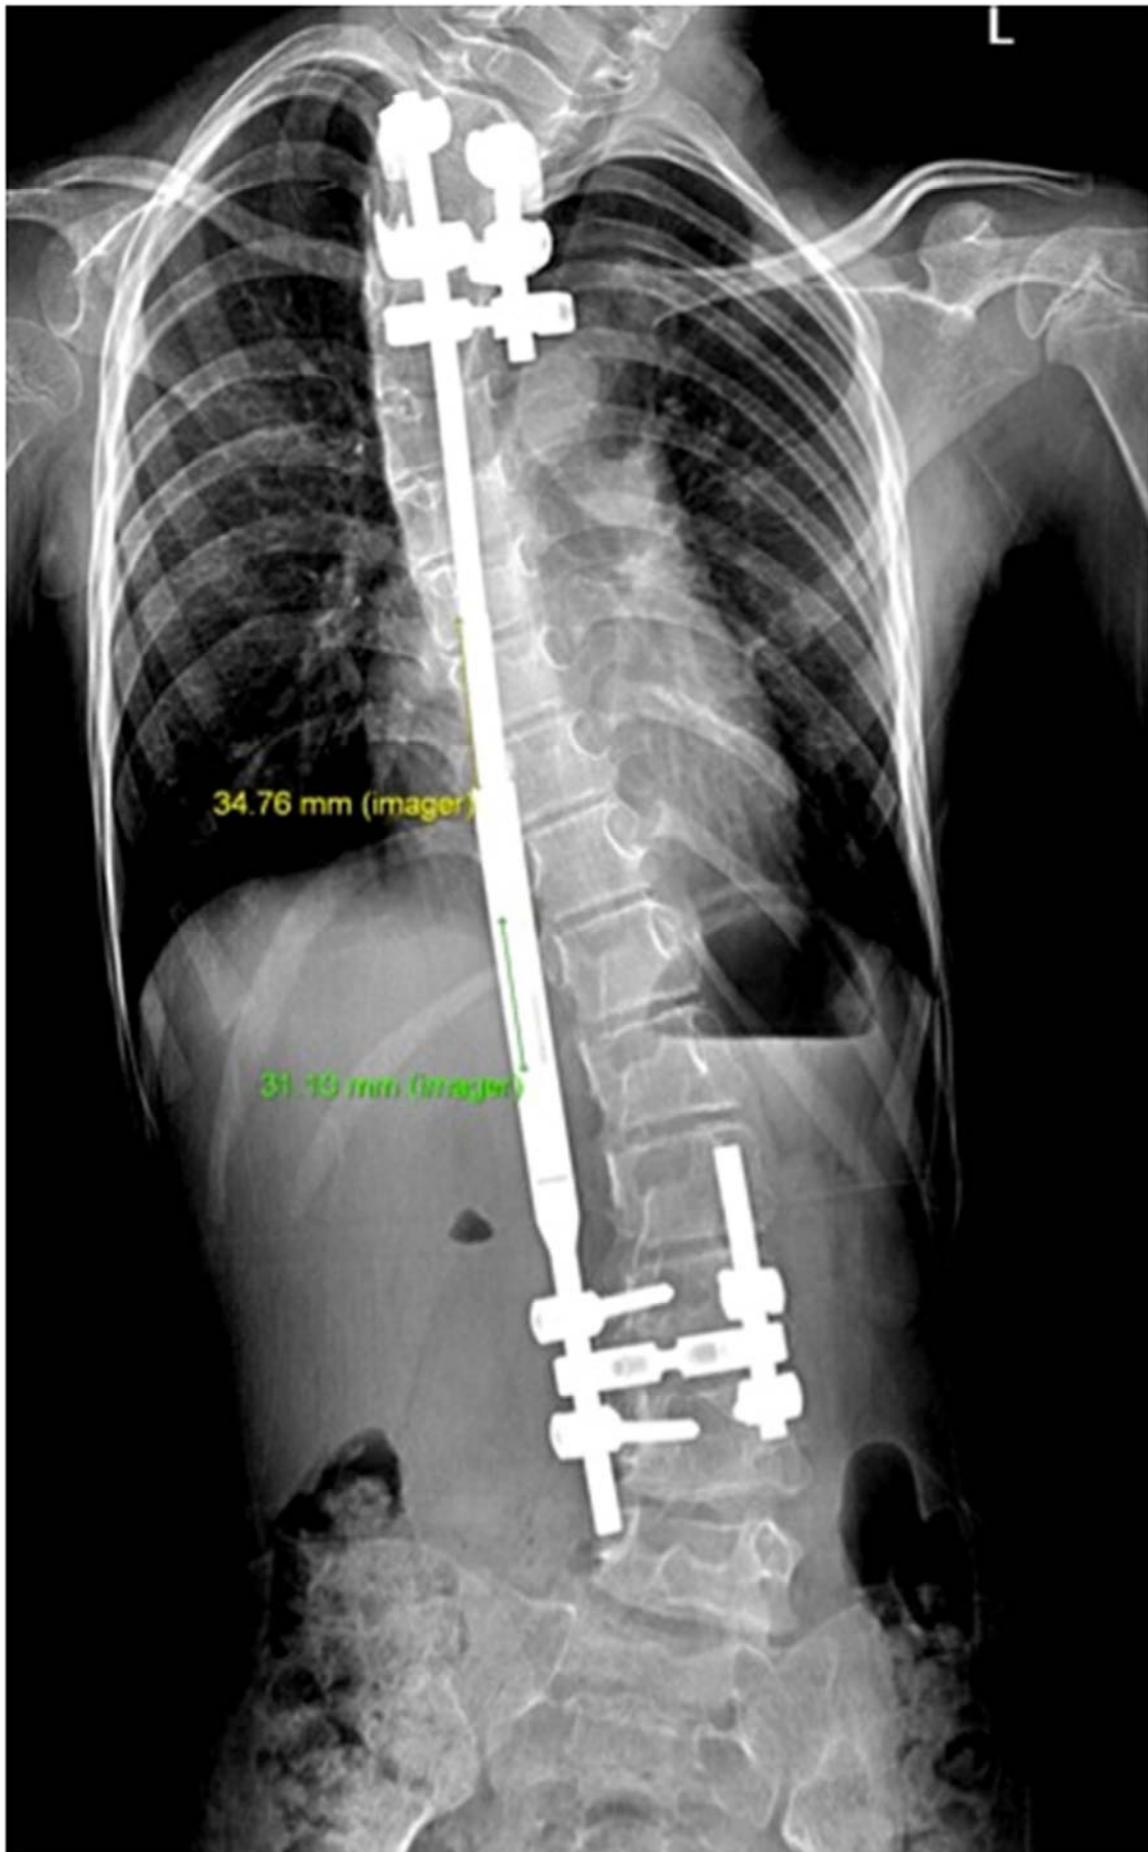

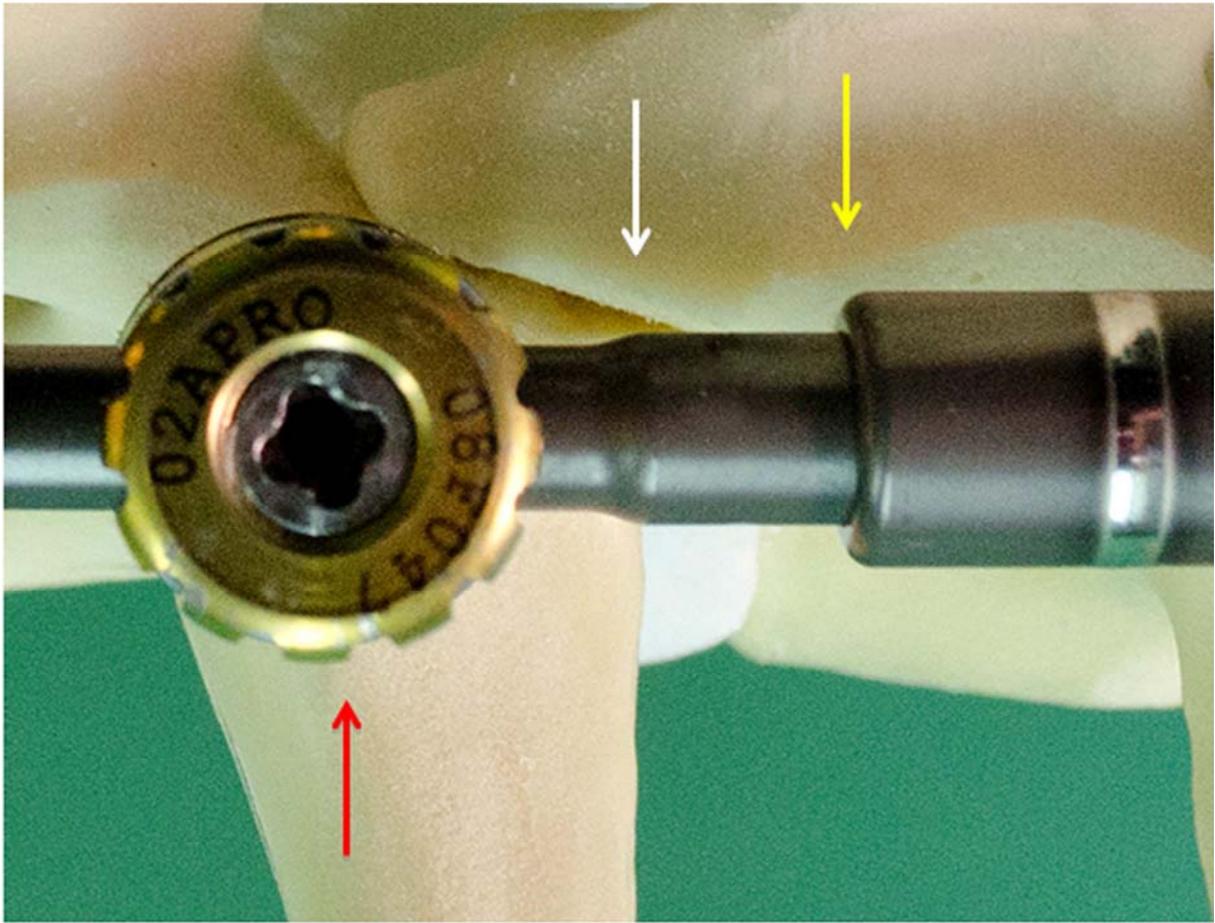


ACCEPTED MANUSCRIPT

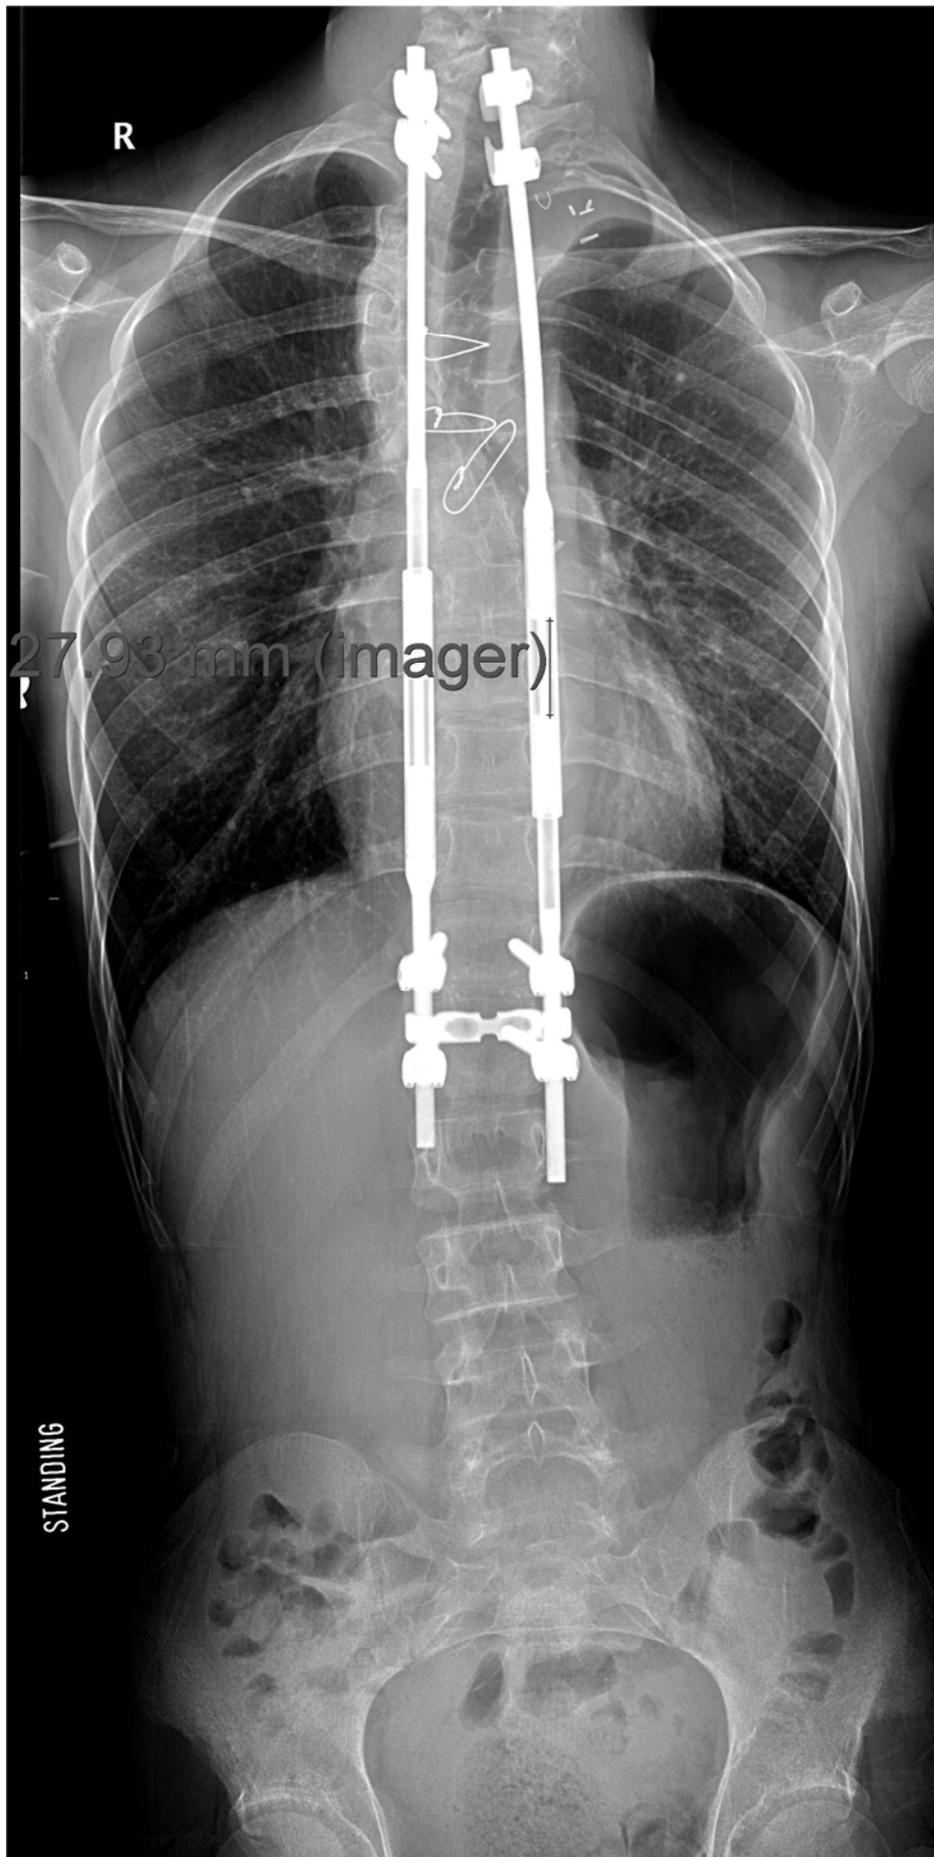



ACCEPTED MANUSCRIPT

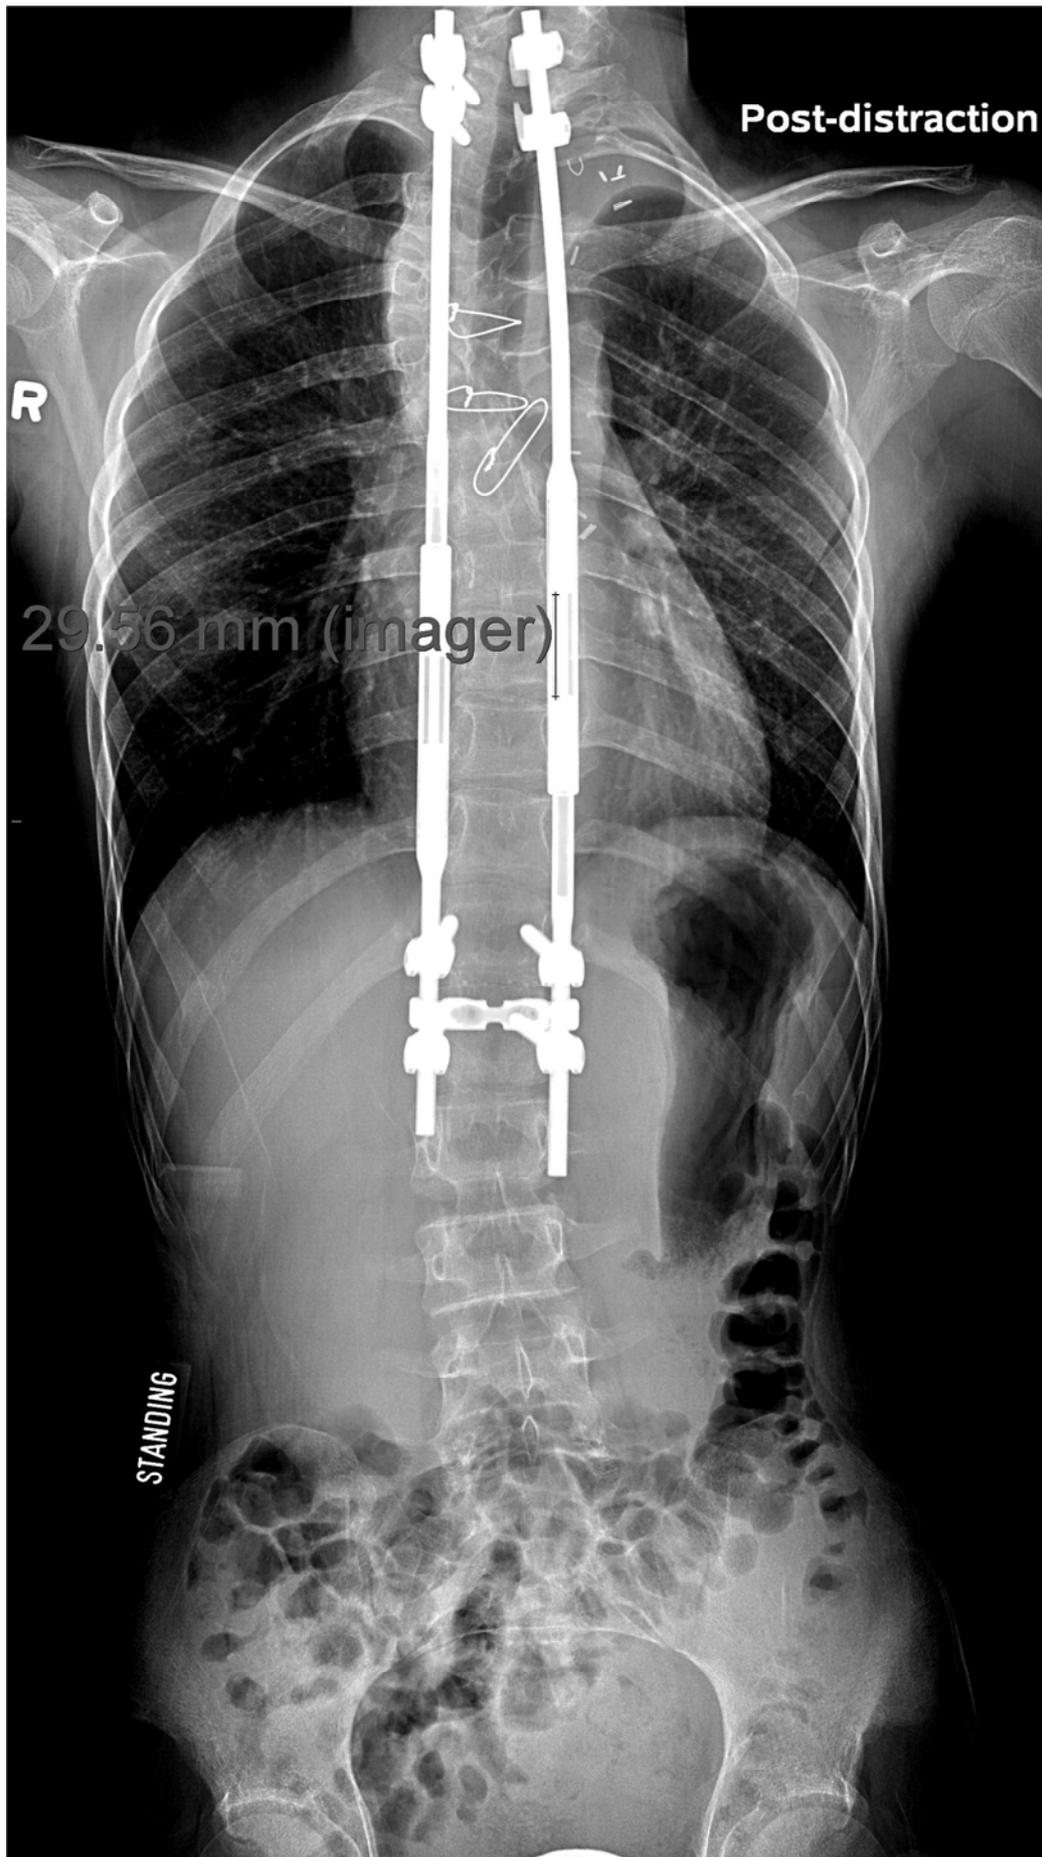



ACCEPTED MANUSCRIPT