



Title	LC decoupling circuit for arbitrarily placed coils
Author(s)	Wu, B; Qu, P; Pang, Y; Shen, GG
Citation	The International Society for Magnetic Resonance in Medicine 14th Scientific Meeting & Exhibition (ISMRM2006). Seattle, WA, 6-12 May 2006, p. 3522
Issued Date	2006
URL	http://hdl.handle.net/10722/98904
Rights	This work is licensed under a Creative Commons Attribution- NonCommercial-NoDerivatives 4.0 International License.

LC Decoupling Circuit for Arbitrarily placed Coils

B. Wu¹, P. Qu¹, Y. Pang¹, G. X. Shen¹

¹Electrical and Electronics Engineering, The University of Hong Kong, Hong Kong, Hong Kong, Hong Kong

Introduction

The use of coil arrays has become widespread in applications for parallel MRI. The conventional decoupling technique of coil overlap leads to stringent constraints on how the elements are placed. This fixed overlap may not always be appropriate for parallel spatial encoding [1]. Some alternative decoupling methods are to insert capacitors or LC circuit networks between coils to minimize their mutual coupling [2-7]. To clearly illustrate the LC decoupling circuit, the technique by inserting decoupling-capacitors (C_d) or decoupling-inductors (L_d) for isolation arbitrary-placed coils was studied. Also we compared the decoupling performance by using C_d and L_d at different magnetic strengths.

Method

(1) Two coupled cases: The coupled coils can be simplified into two cases according to the current direction in each loop, i.e. the currents in primary and secondary coils have the opposite direction, thus the voltage in secondary coil increases caused by the induced current. In this case, the mutual coupling M has positive sign ($M>0$). On the contrary when the currents in primary and secondary coils have the same direction, $M<0$. Two typical examples are listed in fig.1. In fig.1a, when the angle between two loops are larger to 90° (a1), or the two coplanar loops are overlapped too less than the exact overlap, or separated without any overlap (a2), $M>0$. On the contrary, when angle between loops are less than 90° (b1), or the two loops are overlapped too much (b2), $M<0$.

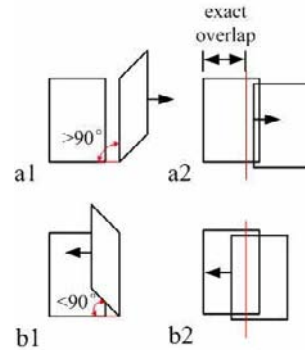


Fig.1. The two coupling cases. a1 and a2: $M>0$. b1 and b2: $M<0$.

(2) Decoupling LC circuit for $M>0$ and $M<0$: To illustrate the decoupling circuit more clearly, four decoupling methods are applied on loop pair which are overlapped too less (Fig.2a) and overlapped too much (Fig.2b). C_1 is the tuning capacitor defined as the figure shows. C_2 is the equivalent capacitors except C_1 . These methods can be explained by vector analysis [6]. Fig.3a illustrates the methods in fig.2a1-a4 and fig.3b illustrates the methods in fig.2b1-b4. I_i represents the induced current in the second coil, I_d is the additional current introduced by decoupling circuits to diminish I_i . I_i represents the induced current after decoupling. θ is the loss angle of the sample and δ is the loss angle caused by C_d or L_d .

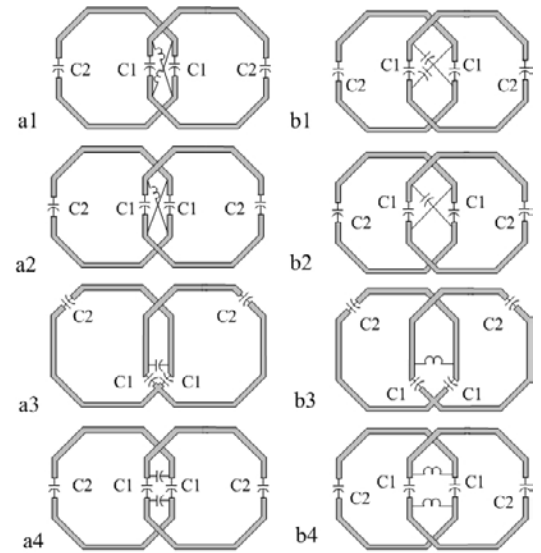


Fig.2. Coil pairs which are overlapped too less (a) and overlapped too much (b) are used to illustrate the decoupling techniques. Four circuits for each case are shown in 1-4.

Result

(1) C_d and L_d vs. resonant frequency: According to analysis models we established, relationships of the required C_d and L_d vs. resonant frequency are shown in fig.4. L represents the self-inductor of each coil. For the method by using inductors (in fig. 2. a1, a2, b1, b2), L_d is proportional to L . When the material and geometry of coils are fixed, L_d is independent of resonant frequency (fig.4c and d). While for decoupling capacitors (in fig.2. a3, a4, b3, b4), C_d is proportional to $1/(L\omega^2)$ (fig.4a and b). Thus at ultra-high-field or very-low-field system, L_d is easier to implement than C_d since in these frequency ranges, the value of C_d is sometimes with unreasonable value for choosing.

(2) Coil isolation and SNR by using C_d and L_d : According to fig.3, the loss of the inserting circuits can decrease the coil isolation. Due to δ of L_d is usually larger than that of C_d , at low field when coil loss is dominant, the isolation and SNR by using C_d is better than L_d . While at high field when sample loss dominant ($\theta > \delta$), both methods by using L_d and C_d have the similar performance.

Conclusion

The LC circuits in fig.2 can be used to isolate coil pairs and can be extended to decouple arbitrarily placed multiple coils by inserting the LC circuit between each pair. At low field, C_d can provide better isolation than L_d . At high field, method by using L_d is an alternative of C_d .

Reference

[1].Weiger M. et al., MRM 2001:495-504. [2] T.T.Fox. SMRM, 1989:99. [3] J.Wang. ISMRM 1996:1434. [4]. J. Lian, P.B.Roemer, US Patent #5,804,969. [5]. J.Jevic, ISMRM 2001:17. [6].Zhang X, Webb A. JMR 2004:149-155. [7].R.F.Lee et al., MRM 2002:203-213.

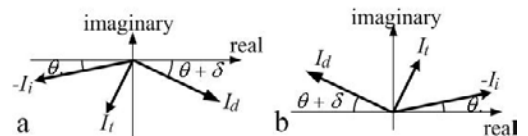


Fig.3. Vector analysis of the decoupling techniques. The explanation of the case when $M>0$ (fig.3a) and the case when $M<0$ (fig.3b)

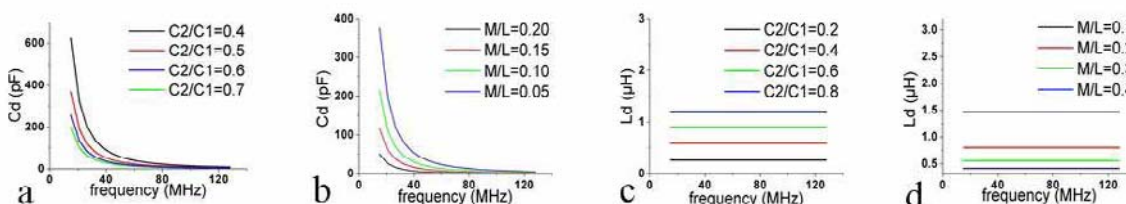


Fig.4. Relationships of L_d and C_d vs. frequency. Assuming $L=0.5\mu\text{H}$. M is absolute value of mutual inductance. In a and c, set $M/L=0.1$. In b and d, set $C_2/C_1=1$.